

FIG. 1

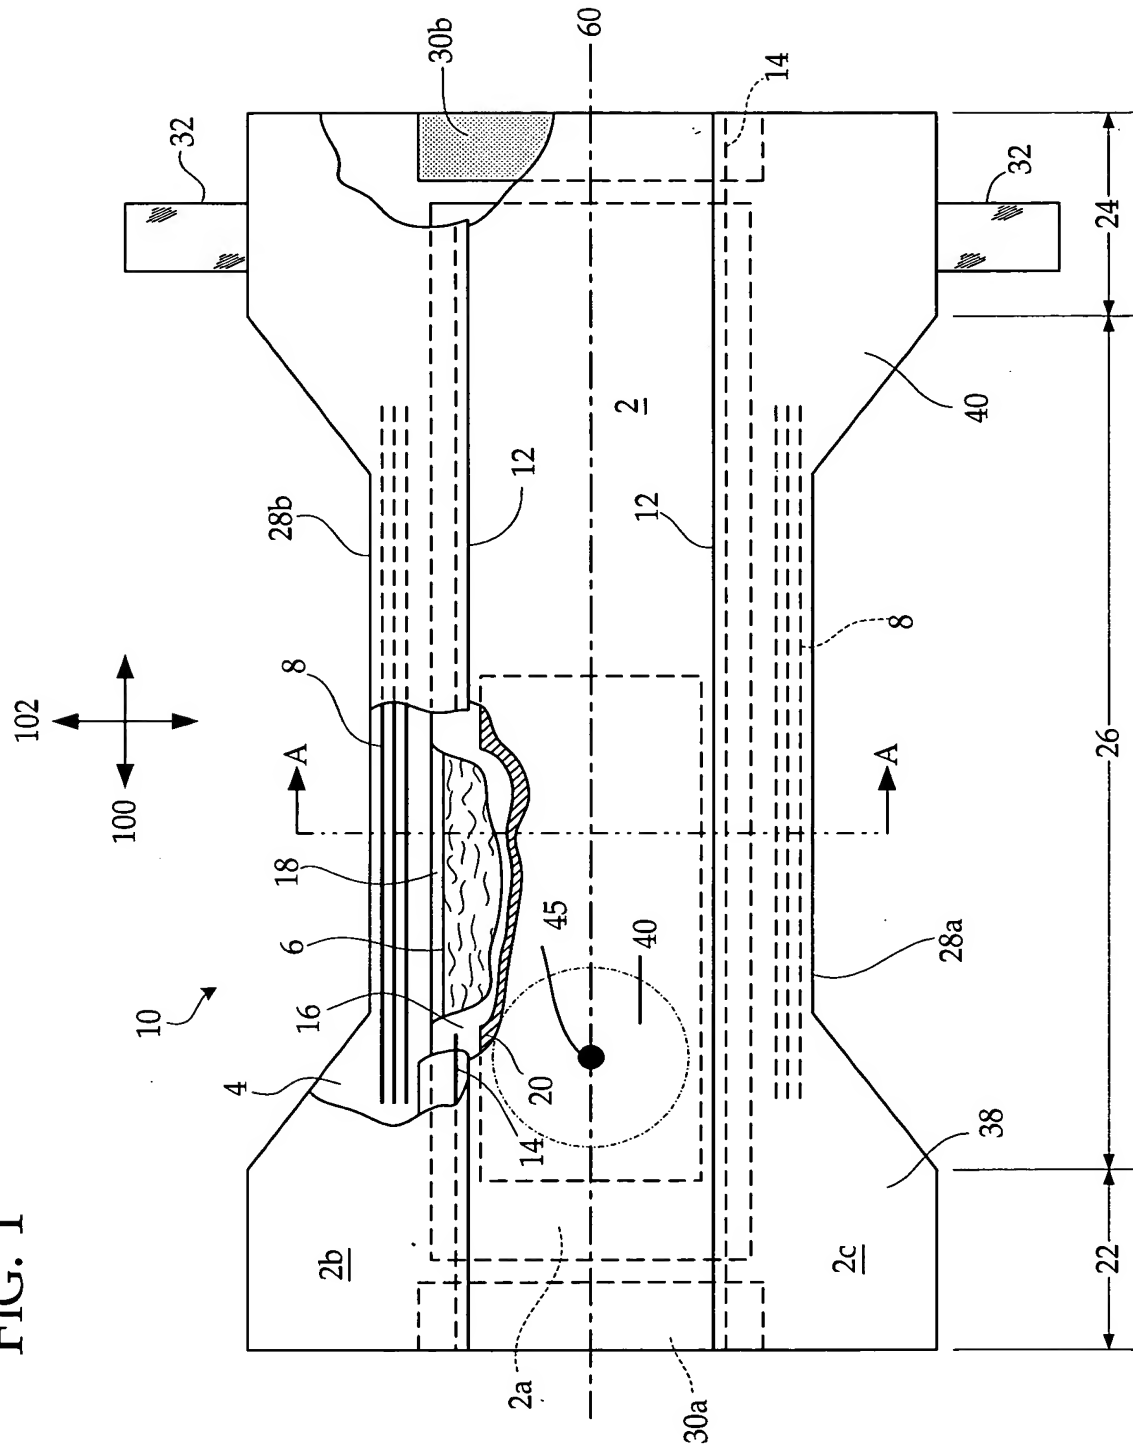


FIG. 2

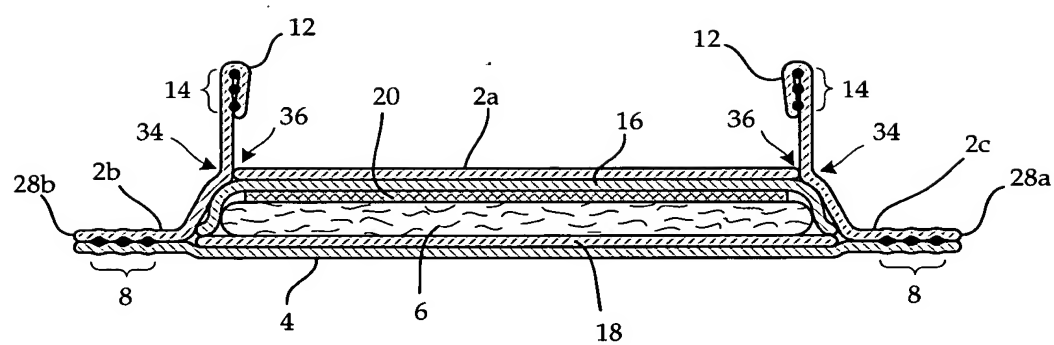


FIG. 3

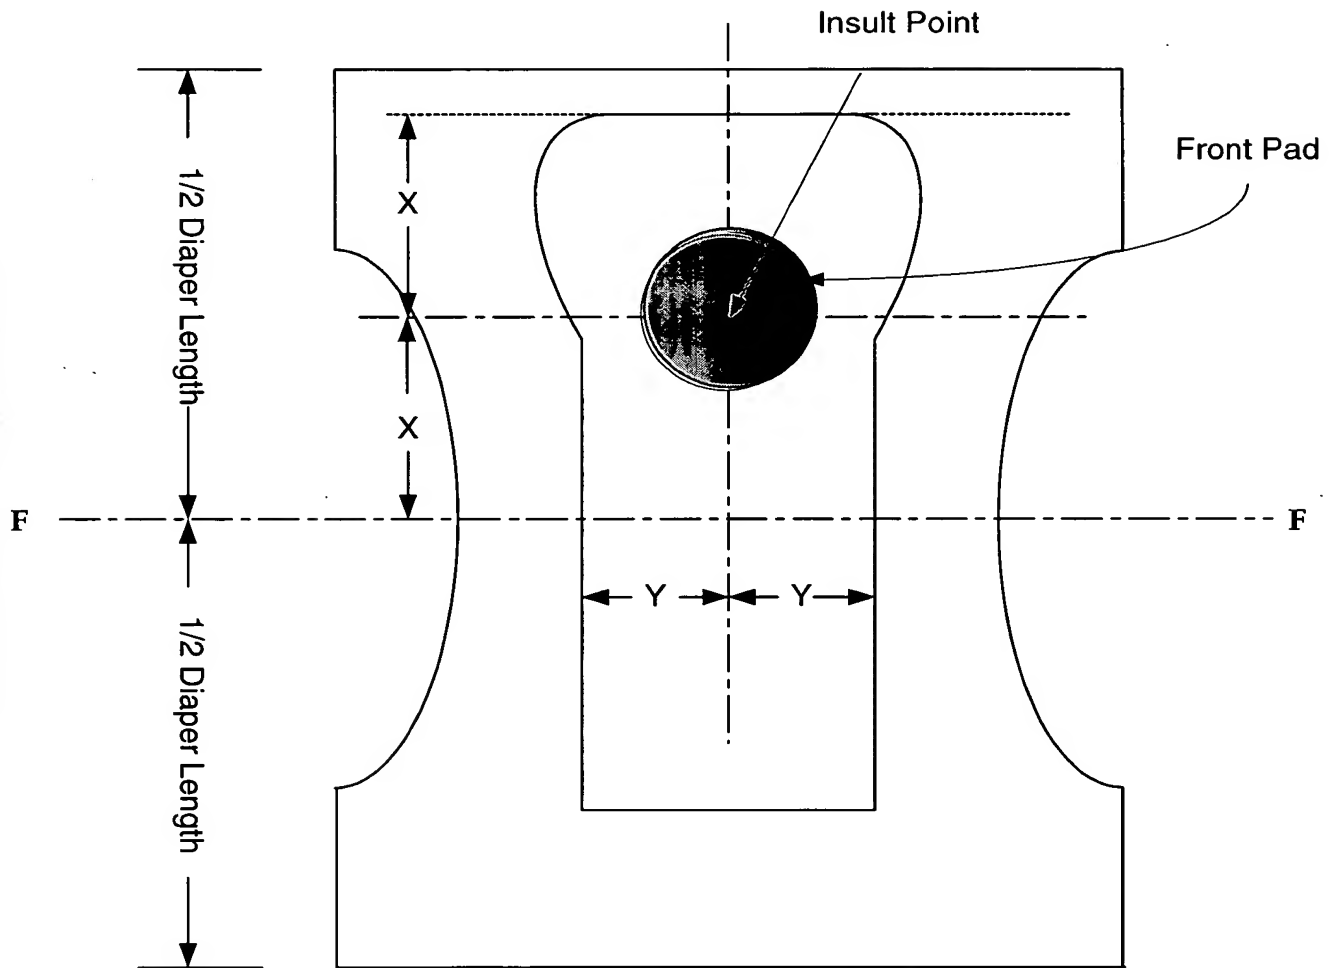


FIG. 4

2025065 012902


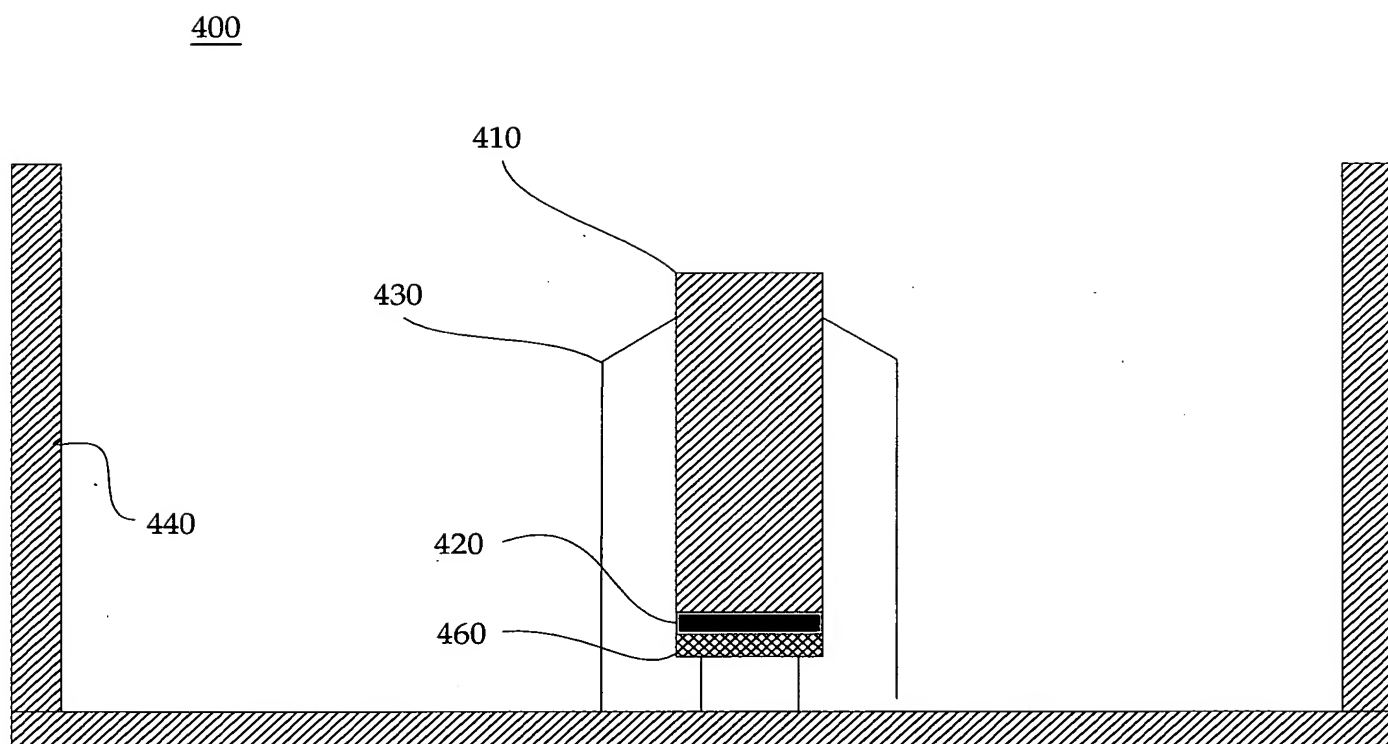


FIG. 5

10058065, 012302

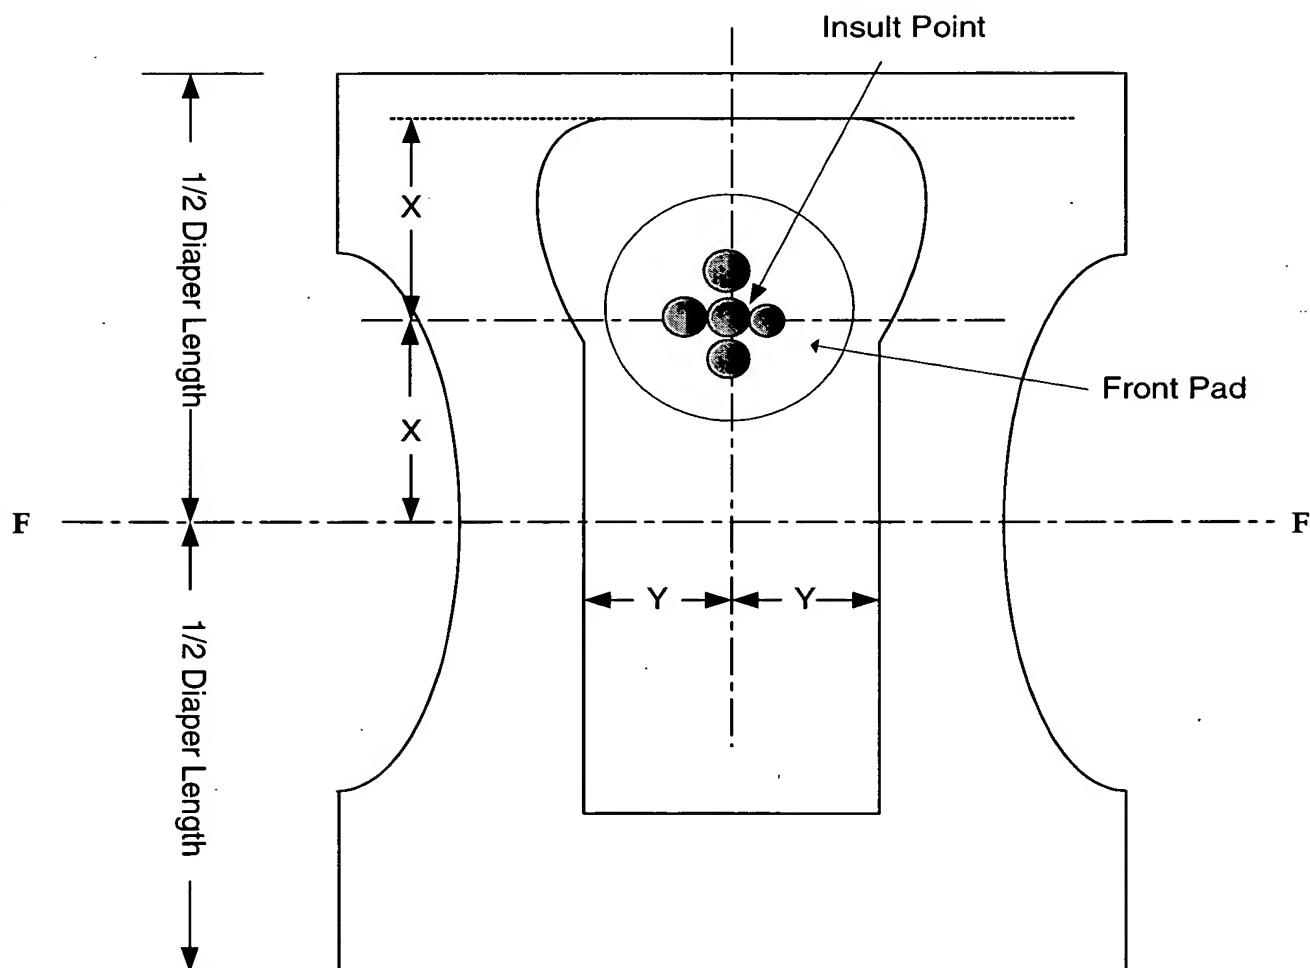

TOTAL FRONT PAD CAPACITY v. Urine Leakage

(1.0% NaCl Solution, 10 minutes exposure, 0.5 psi restraining pressure)

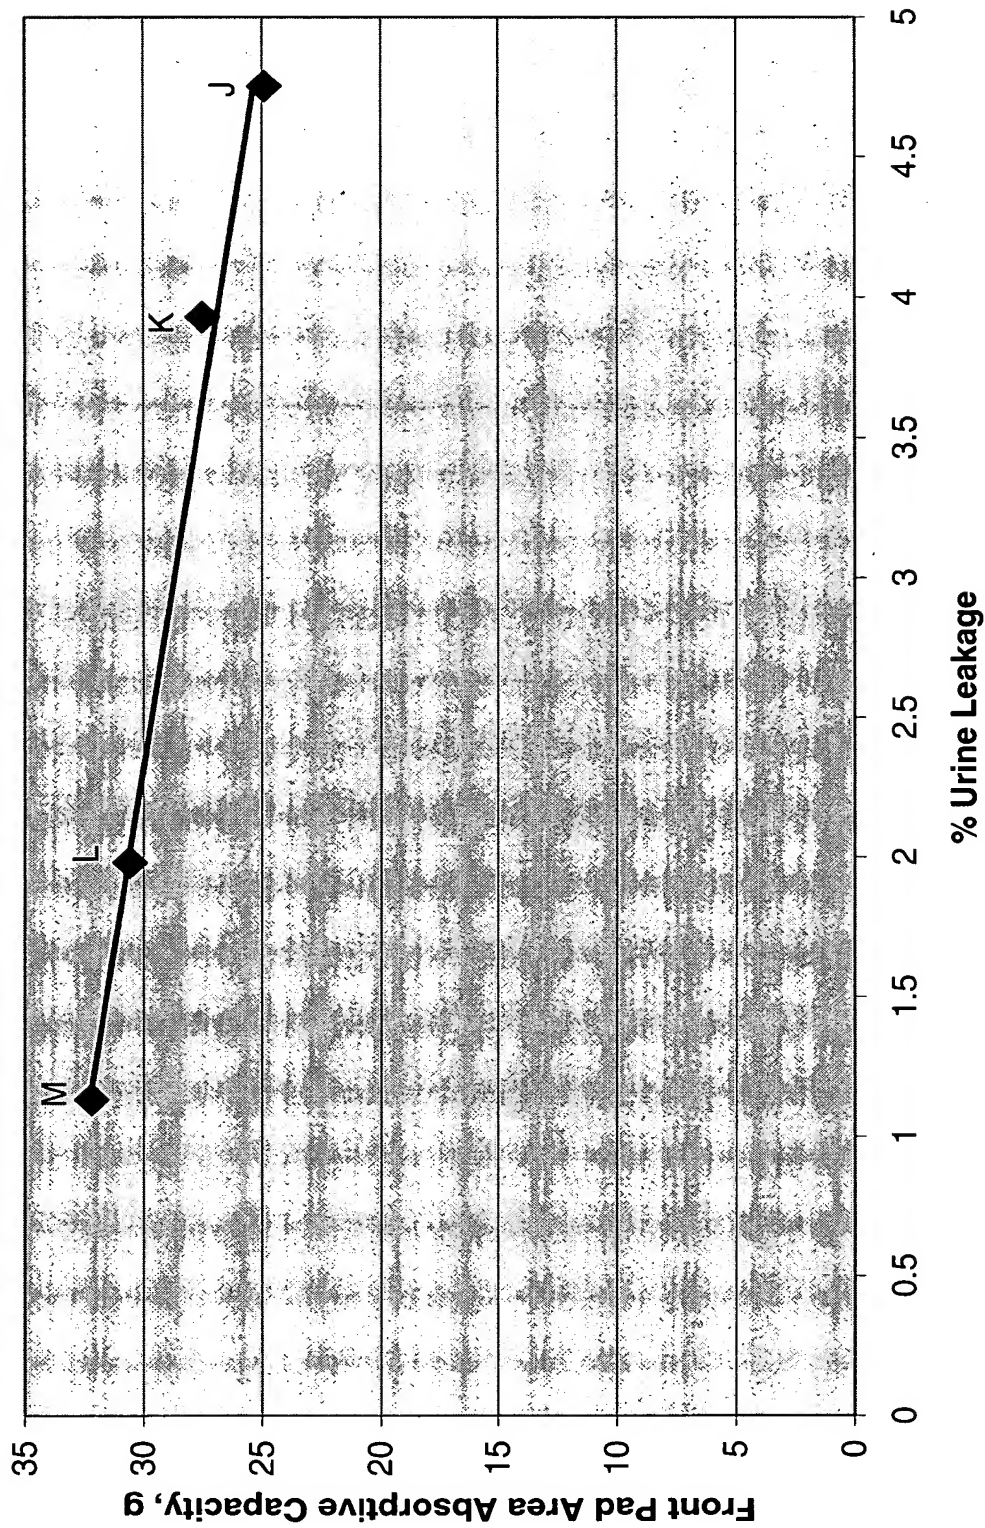


FIG. 6